

FEATURES

High precision High efficiency High output voltage stability Linear modulation of output voltage Low cost Overcurrent protection Short circuit protection Digital display for output voltage

APPLICATIONS

AHVACN5KV1MABT, is designed for achieving AC-DC conversion from AC voltage to high DC voltage. High voltage power supply is widely used in industrial measurement and control, energy spectrum analysis, and medical equipment such as: X-ray machine, vacuum/plasma processing, semiconductor fabrication equipment, analytical instrumentation, medical diagnostic and therapeutic systems, test equipment, and research and academic applications, etc. **DESCRIPTION**

Connect AC 100~240V input, and then power on. When the potentiometer is in "0", open the high voltage switch, and then adjust the potentiometer clockwise. Observe the digital

display readings, and high voltage power supply output voltage = the reading \times 10V. When the required voltage is achieved, then rotate the potentiometer lock clockwise to lock the potentiometer. This prevents the output voltage changes caused by rotating the potentiometer by accident. High voltage connection wire is used for high voltage output.

SAFETY PRECAUTIONS

High voltage power supply must be connected to ground reliably.

Do not touch the high voltage wire, unless the high voltage power supply is powered off, and the load and internal capacitors are fully discharged.

When the high voltage power supply is powered off, wait for another 5 minutes for fully discharging all the capacitors inside the power supply.

Do not operate the power supply in humid environment, and do not connect the operator to ground.

The internal protection circuit is provided in the high voltage power supply, but the high voltage short circuit shall be avoided.

Make sure the circuit is insulated perfectly, especially between the high voltage output and the surroundings so as to avoid electronic shock.

©Copyrights 2000-2021, Analog Technologies, Inc. All Rights Reserved. Updated on 3/3/2021 Email: staff@analogti.com/sales@analogti.com 1



SPECIFICATIONS

Table 1. Characteristics.

 $T_A = 25$ °C, unless otherwise noted

Parameter		Symbol	Condition	Min.	Тур.	Max.	Unit/Note
AC Inp	out Voltage	VPS		100	110	240	V _{AC}
Quiescent	Input Current	I _{INQQ}	$I_{OUT} = 0mA$	22	27	32	mA
Full Load	Input Current	I _{INFLD}	$I_{OUT} = 1.0 mA$	80	85	90	mA
Input Voltage	Regulation Ratio	$\Delta V_{OUT} / \Delta VPS$	$VPS = 100V \sim 240V$		0.5		%
Outp	ut Voltage	V _{OUT}	$I_{OUT} = 0 \sim 1.0 \text{mA}$	0		-5000	V
Maximum	Output Current	I _{OUTMAX}	$VPS = 100V \sim 240V$			1.0	mA
I	Load				5		MΩ
Potentiome	eter Adjustment			10k potentiometer			
Output Mod	ulation Linearity			<1		%	
Load Reg	gulation Rate		$I_{OUT} = 0 \sim 1.0 \text{mA}$	≤0.05		%	
Instantaneous S	hort Circuit Current	I _{SC}		<20		mA	
Full Loa	Full Load Efficiency				≥70		%
Temperatu	re Coefficient	TCVo	−20 ~ 50°C		< 0.05		%/°C
	Short Time Drift				< 0.5		%/ min
Time Drift	Long Time Drift				<1		%/h
Output Voltage T	Cemperature Stability		−20 ~ 50°C	< <u>±1</u>		%	
Operating Temperature Range		T _{opr}		-10		55	°C
Storage Temperature Range		T _{stg}		-25		65	°C
External Dimensions				180×120×50		mm	
Weight					1192		g
					2.63		lbs
					42.05		Oz



High Voltage Power Supply AHVACN5KV1MAB

PANEL INSTRUCTIONS

Left Panel




Figure 2. Left Panel

1. HV output: 1m long connection wire outputs -5kV 1MA.

2. Output ground: high voltage power supply output ground terminal.

Front Panel



Figure 3. Front Panel

3. Output display: Digital display for output voltage. The actual output voltage = display reading $\times 10$ V.

4. HV adjustment: 10-turn potentiometer for adjusting output voltage. Rotate it clockwise to increase the output voltage, and the potentiometer resistance = the corresponding scale × 10 Ω . For example, as Figure 4 shows, when the scale is 10, and the frame above the scale shows 1 (1k Ω), then the resistance =10×10 Ω +1k Ω =1.1k Ω , and the like.



Figure 4. Scale and Resistance Calculation

5. High voltage ON/OFF switch

6. Potentiometer lock: when turn the lock clockwise, then the potentiometer is locked, so that the POT will not be rotated for any voltage change.

Right Panel

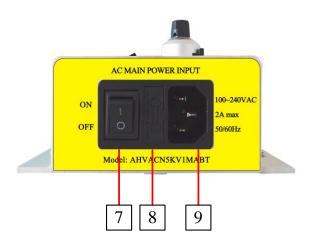


Figure 5. Right Panel

- 7. Main power ON/OFF switch
- 8. Fuse: 250V/2A
- 9. Input connector: AC input 100 ~ 240 50/60Hz connector.


1161 Ringwood Ct, #110, San Jose, CA 95131, U. S. A. Tel.: (408) 748-9100, Fax: (408) 770-9187

3

©Copyrights 2000-2021, Analog Technologies, Inc. All Rights Reserved. Updated on 3/3/2021 Email: staff@analogti.com/sales@analogti.com/



TESTING DATA

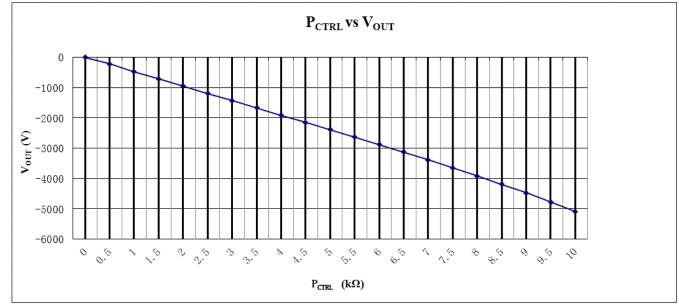

High voltage power supply testing data (Test condition: the load is 5 $\ensuremath{M\Omega}\xspace$)

NAMING INSTRUCTIONS

		<u>N AC N</u>	5KV 1 MA B	T		
Company code: Analog Technologies, Inc.	Product type: High Voltage Power Supply	Polarity N = negative P = positive	Max. Out Voltage 100V=100V 5KV=5kV 10KV=10kV	R5 = 0.5	Ont.	Type: BT = Bench top

Figure 7.	Naming	Rules of	AHVACI	N5KV1MABT
-----------	--------	----------	--------	-----------

©Copyrights 2000-2021, Analog Technologies, Inc. All Rights Reserved. Updated on 3/3/2021 Email: staff@analogti.com/sales@analogti.com 4

Figure 6. P_{CTRL} vs. V_{OUT}



High Voltage Power Supply

AHVACN5KV1MAB

DIMENSIONS


I. Dimension of the leads.




Figure 8. Leads of AHVACN5KV1MABT

Leads	Diameter (mm)	Length (m)		
Thick brown lead	4.5	1.0		
Power cord	6.5	1.8		

II. Dimension of AHVACN5KV1MABT.

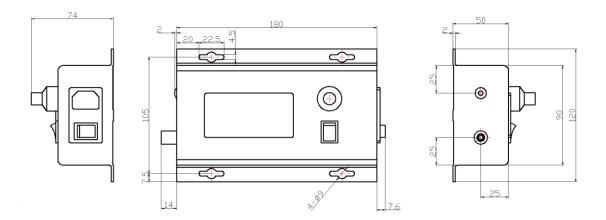





PRICES

Quantity (pcs)	1~9	10~49	50~99	≥100
AHVACN5KV1MABT	\$389	\$379	\$369	\$359

NOTICE

- 1. ATI warrants performance of its products for one year to the specifications applicable at the time of sale, except for those being damaged by excessive abuse. Products found not meeting the specifications within one year from the date of sale can be exchanged free of charge.
- 2. ATI reserves the right to make changes to its products or to discontinue any product or service without notice, and advise customers to obtain the latest version of relevant information to verify, before placing orders, that information being relied on is current and complete.
- 3. All products are sold subject to the terms and conditions of sale supplied at the time of order acknowledgment, including those pertaining to warranty, patent infringement, and limitation of liability. Testing and other quality control techniques are utilized to the extent ATI deems necessary to support this warranty. Specific testing of all parameters of each device is not necessarily performed, except those mandated by government requirements.
- 4. Customers are responsible for their applications using ATI components. In order to minimize risks associated with the customers' applications, adequate design and operating safeguards must be provided by the customers to minimize inherent or procedural hazards. ATI assumes no liability for applications assistance or customer product design.
- 5. ATI does not warrant or represent that any license, either express or implied, is granted under any patent right, copyright, mask work right, or other intellectual property right of ATI covering or relating to any combination, machine, or process in which such products or services might be or are used. ATI's publication of information regarding any third party's products or services does not constitute ATI's approval, warranty or endorsement thereof.
- 6. IP (Intellectual Property) Ownership: ATI retains the ownership of full rights for special technologies and/or techniques embedded in its products, the designs for mechanics, optics, plus all modifications, improvements, and inventions made by ATI for its products and/or projects.